

==== Shimadzu LabSolutions Analysis Report =====

Sample Name : PH_20PureAcetol_220C_041125_8
 Sample ID :
 Data Filename : PH_20PureAcetol_220C_041125_8_20251104_PH_20PureAcetol_220C_SFB_B_ST1_
 Method Filename : SFB_B_ST1_0.8 mL_45 min_Start.lcm
 Batch Filename : 20251104_PH_20PureAcetol_220C.lcb
 Vial # : 2-36 Sample Type : Unknown
 Injection Volume : 10 uL
 Date Acquired : 11/6/2025 12:45:53 PM Acquired by : System Administrator
 Date Processed : 11/6/2025 1:30:53 PM Processed by : System Administrator

<Method>

<<Header>>

Generated : 4/24/2024 3:47:23 PM
 GeneratedBy : System Administrator
 Modified : 11/5/2025 8:17:40 AM
 ModifiedBy : System Administrator

<<System Controller>>

Model : SCL-40
 Event1 : Off
 Event2 : Off
 Sample Load Timing : Off

<<Data Acquisition>>

LC Stop Time : 45.00 min
 Detector A Name : Detector A
 Detector A Sampling Frequency : 2 Hz
 Detector A Start Time : 0.00 min
 Detector A End Time : 45.00 min

<<Pump>>

Mode : Isocratic flow
 Pump A : LC-40D
 Pump A Flow/Pressure : Flow
 Pump System A Flow : 0.8000 mL/min
 Pump System A Flow Slope : 20.00 min
 Pump A PressMax : 90 bar
 Pump A PressMin : 0 bar
 Pump A Valve Model : Switching Valve
 Pump A Valve : B
 Pump A Compressibility Setting : On
 Pump A Mobile Phase Settings : 0.45 /GPa

<<Autosampler>>

Autosampler Model : SIL-40
 Enable Autosampler : Use
 Rinse Type : External only
 Specify Plate : Off
 Rinsing Volume : 500 uL
 Cut Off Loop : Off
 Specify Needle Stroke : Off
 Rinsing Speed : 35 uL/sec
 Sampling Speed : 5.0 uL/sec
 Rinse Port R0 Purge Time : 2.0 min
 Measuring Line Purge Time : 5.0 min
 Rinse Mode : Before and after aspiration
 Rinse Dip Time : 0 sec
 Measuring Line Purge Volume : 100 uL
 Air Gap Volume : Off
 Rinse Port Liquid : R0

<<Sample Pretreatment>>

Mode : Standard

<<Oven>>

Oven Model : CTO-40C
 Enable Oven : Use
 Oven Temperature : 25 C
 Maximum Temperature : 105 C

Ready Check	: On
Wait Time	: 5 min
Ready Range	: 1.0 C
Fan Speed	: Auto
Cooler Mode	: Auto
Valve 1/L	: FCV-0206
Valve 1/L Position	: 1

<<Detector A>>

Model	: RID-20A
Mode	: Analytical
Polarity	: +
Use Cell Temp.	: Use
Cell Temp.	: 40.0 C
Response	: 1.5 sec
Intensity Unit	: Volt
Auxiliary Range	: 1.0E-3 RIU/V
Recorder Range	: 100.00 uRIU/FS
Synchronize with Auxiliary	: Off
Purge Time	: 20 min

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	RID-20A(DET.A)	Zero		
45.00	Controller	Stop		

<<Peak Integration>>

<Detector A>

```

Detector Type      : 1
Channel            : Ch1
Width              : 5 sec
Slope              : 2000 uV/min
Drift              : 0 uV/min
T.DBL              : 1000 min
Max Slices         : 0
Peak Top Detection : Normal
RT Compensation Mode : Fine
Min.Area/Height is made effective in Manual Integration : Off
Min.Area/Height    : 1000 counts
Calculated by       : Area
Noise Calculation Settings : Noise Data : Current Data
                               Calculation Method : ASTM
                               Range : Whole Range
                               Interval : 0.5 min
                               Include the Peak Detected Range : Off
                               Detection Limit Coefficient : 3.3
                               Quantitative Limit Coefficient : 10.0
Drift Calculation Settings : 0.000 - 15.000 min

```

<<Integration Time Program(Method)>>

<Detector A>

Channel : Ch1
Time Program : None

<<Integration Time Program(Data)>>

<Detector A>

Channel : Ch1
Time Program : None

<<Identification>>

<Detector A>

Window/Band	: Window
Window	: 5.00 %
Identification Method	: Absolute
Peak Selection	: Closest Peak
Display not identified peaks	: Not display

<<Quantitative>>

<Detector A>

Quantitative Method	: External Standard
Calculated by	: Area
# of Calibration Levels	: 14
Curve Fit Type	: Linear
Zero	: Not Forced
Weighting Method	: None
X Axis of Calib. Curve	: Conc.
Units	: mol/L
Format of Conc.	: Decimals
Format of Conc. Figure	: 5
Group Type	: Not Used

Check %Dev(Standard) : No
 Check Accuracy[%](Standard) : No
 Check %Dev(Control) : No
 Check Accuracy[%](Control) : No
 Check %Dev(Additive) : No
 Check Accuracy[%](Additive) : No
 Check %Dev(Unknown) : No
 Check Accuracy[%](Unknown) : No
 Check Quantitation Limit : No
 Check Detect Limit : No

<<Compound Table>>

<Detector A>

ID# : 1
 Name : Methanol
 Type : Target
 Channel : Ch1
 Retention Time : 14.400 min
 Retention Index : 0
 Concentration : [1]=3.016738 [2]=1.049395 [3]=0.4943277
 [4]=0.2893701 [5]=0.1127578 [6]=0.06136267
 [7]=0.01619725 [8]=3.016738 [9]=1.049395
 [10]=0.4943277 [11]=0.2893701 [12]=0.1127578
 [13]=0.06136267 [14]=0.01619725
 Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 4.720087e+005
 Intersection : 1.693726e+003
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 2
 Name : Glycerin
 Type : Target
 Channel : Ch1
 Retention Time : 10.000 min
 Retention Index : 0
 Concentration : [1]=2.958375 [2]=1.078646 [3]=0.5353454
 [4]=0.3066948 [5]=0.114594 [6]=0.05901699
 [7]=0.0117174 [8]=2.958375 [9]=1.078646
 [10]=0.5353454 [11]=0.3066948 [12]=0.114594
 [13]=0.05901699 [14]=0.0117174
 Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 7.326784e+006
 Intersection : 2.573900e+005
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 3
 Name : n-Propanol
 Type : Target
 Channel : Ch1
 Retention Time : 20.000 min
 Retention Index : 0
 Concentration : [1]=3.02526 [2]=1.092217 [3]=0.5139845
 [4]=0.3105323 [5]=0.09785473 [6]=0.04497364
 [7]=0.01087275 [8]=3.02526 [9]=1.092217
 [10]=0.5139845 [11]=0.3105323 [12]=0.09785473
 [13]=0.04497364 [14]=0.01087275
 Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 3.955755e+006
 Intersection : -2.585461e+004

Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 4
 Name : 1,2 Propandiol
 Type : Target
 Channel : Ch1
 Retention Time : 12.400 min
 Retention Index : 0
 Concentration : [1]=2.977546 [2]=1.016412 [3]=0.5030017
 [4]=0.3027638 [5]=0.1023958 [6]=0.04970167
 [7]=0.01157971 [8]=2.977546 [9]=1.016412
 [10]=0.5030017 [11]=0.3027638 [12]=0.1023958
 [13]=0.04970167 [14]=0.01157971

Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 5.771075e+006
 Intersection : 6.007717e+004
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 5
 Name : 1,3 Propandiol
 Type : Target
 Channel : Ch1
 Retention Time : 13.000 min
 Retention Index : 0
 Concentration : [1]=2.976375 [2]=0.9968958 [3]=0.4990984
 [4]=0.2900131 [5]=0.10734 [6]=0.04944145
 [7]=0.0100184 [8]=2.976375 [9]=0.9968958
 [10]=0.4990984 [11]=0.2900131 [12]=0.10734
 [13]=0.04944145 [14]=0.0100184

Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 5.532080e+006
 Intersection : 6.014722e+004
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 6
 Name : iso-Propanol
 Type : Target
 Channel : Ch1
 Retention Time : 16.825 min
 Retention Index : 0
 Concentration : [1]=3.03666 [2]=1.003405 [3]=0.5418687
 [4]=0.3101858 [5]=0.1067771 [6]=0.04972951
 [7]=0.01397083 [8]=3.03666 [9]=1.003405
 [10]=0.5418687 [11]=0.3101858 [12]=0.1067771
 [13]=0.04972951 [14]=0.01397083

Peak Selection : Default(Closest Peak)
 Calculated by : Default(Area)
 Curve Fit Type : Default(Linear)
 Zero : Default(Not Forced)
 Weight : Default(None)
 Window/Band : Default(Window)
 Spiked : 0.000
 1st Coefficient : 3.797216e+006
 Intersection : -2.284739e+004
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000

ID# : 7
 Name : Hydroxyacetone
 Type : Target
 Channel : Ch1
 Retention Time : 13.300 min
 Retention Index : 0
 Concentration : [1]=2.855514 [2]=0.9609004 [3]=0.4875675

	[4]=0.3072624	[5]=0.1038742	[6]=0.04860286
	[7]=0.009361501	[8]=2.855514	[9]=0.9609004
	[10]=0.4875675	[11]=0.3072624	[12]=0.1038742
	[13]=0.04860286	[14]=0.009361501	
Peak Selection	: Default(Closest Peak)		
Calculated by	: Default(Area)		
Curve Fit Type	: Default(Linear)		
Zero	: Default(Not Forced)		
Weight	: Default(None)		
Window/Band	: Default(Window)		
Spiked	: 0.000		
1st Coefficient	: 4.865699e+006		
Intersection	: 5.855022e+004		
Correction Factor	: 1.000000		
Standard concentration factor	: 1.000000		

ID#	: 8		
Name	: Ethylenglykol		
Type	: Target		
Channel	: Ch1		
Retention Time	: 12.200 min		
Retention Index	: 0		
Concentration	[1]=2.933794	[2]=1.030353	[3]=0.4898163
	[4]=0.3033639	[5]=0.09840986	[6]=0.059971
	[7]=0.01068632	[8]=2.933794	[9]=1.030353
	[10]=0.4898163	[11]=0.3033639	[12]=0.09840986
	[13]=0.059971	[14]=0.01068632	
Peak Selection	: Default(Closest Peak)		
Calculated by	: Default(Area)		
Curve Fit Type	: Default(Linear)		
Zero	: Default(Not Forced)		
Weight	: Default(None)		
Window/Band	: Default(Window)		
Spiked	: 0.000		
1st Coefficient	: 4.284813e+006		
Intersection	: 4.449721e+003		
Correction Factor	: 1.000000		
Standard concentration factor	: 1.000000		

ID#	: 9		
Name	: Ethanol		
Type	: Target		
Channel	: Ch1		
Retention Time	: 16.000 min		
Retention Index	: 0		
Concentration	[1]=3.010594	[2]=1.02339	[3]=0.5257763
	[4]=0.2939754	[5]=0.0961865	[6]=0.04960971
	[7]=0.01299818	[8]=3.010594	[9]=1.02339
	[10]=0.5257763	[11]=0.2939754	[12]=0.0961865
	[13]=0.04960971	[14]=0.01299818	
Peak Selection	: Default(Closest Peak)		
Calculated by	: Default(Area)		
Curve Fit Type	: Default(Linear)		
Zero	: Default(Not Forced)		
Weight	: Default(None)		
Window/Band	: Default(Window)		
Spiked	: 0.000		
1st Coefficient	: 2.109543e+006		
Intersection	: -9.590194e+003		
Correction Factor	: 1.000000		
Standard concentration factor	: 1.000000		

ID#	: 10		
Name	: Propionsäure		
Type	: Target		
Channel	: Ch1		
Retention Time	: 13.600 min		
Retention Index	: 0		
Concentration	[1]=2.962704	[2]=0.9915078	[3]=0.5019324
	[4]=0.3085198	[5]=0.1036906	[6]=0.04835313
	[7]=0.01168534	[8]=2.962704	[9]=0.9915078
	[10]=0.5019324	[11]=0.3085198	[12]=0.1036906
	[13]=0.04835313	[14]=0.01168534	
Peak Selection	: Default(Closest Peak)		
Calculated by	: Default(Area)		
Curve Fit Type	: Default(Linear)		
Zero	: Default(Not Forced)		
Weight	: Default(None)		
Window/Band	: Default(Window)		

Spiked : 0.000
 1st Coefficient : 4.601450e+006
 Intersection : -1.609005e+003
 Correction Factor : 1.000000
 Standard concentration factor : 1.000000


<<Column Performance>>

<Detector A>

Calculation Method : USP
 Unretained Peak Time : Time at 1st Peak
 Column Length : 150 mm
 Calculate Identified Peaks Only : Off
 Calculation of Relative Retention Time : Off

<Chromatogram>

mV

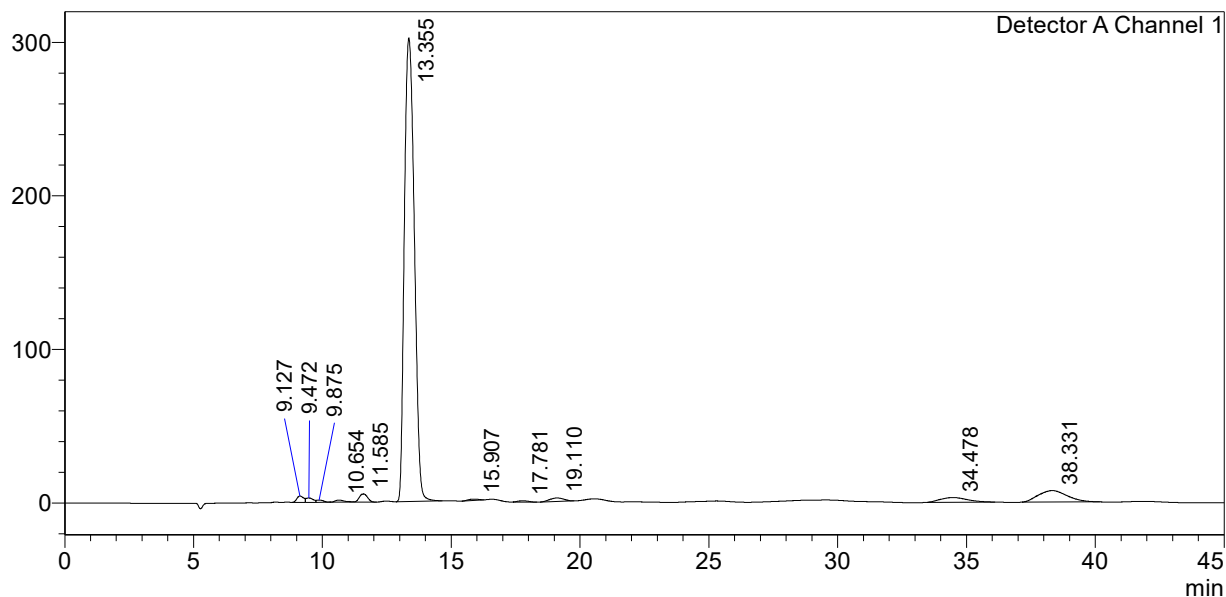

<Peak Table>

Detector A Channel 1

Peak#	Ret. Time	Area	Height	Conc.	Unit	Mark	Name
1	9.127	75513	4103	0.000			
2	9.472	55123	2803	0.000		V	
3	9.875	27256	1442	-0.031	mol/L	V	Glycerin
4	10.654	37682	1403	0.000			
5	11.585	118212	5338	0.027	mol/L	V	Ethylenglykol
6	13.355	8120749	301771	1.657	mol/L		Hydroxyacetone
7	15.907	24933	850	0.016	mol/L		Ethanol
8	17.781	23601	792	0.000			
9	19.110	88911	2281	0.029	mol/L		n-Propanol
10	34.478	222686	3066	0.000			
11	38.331	582992	7469	0.000			
Total		9377658	331317				